



Fig. 1

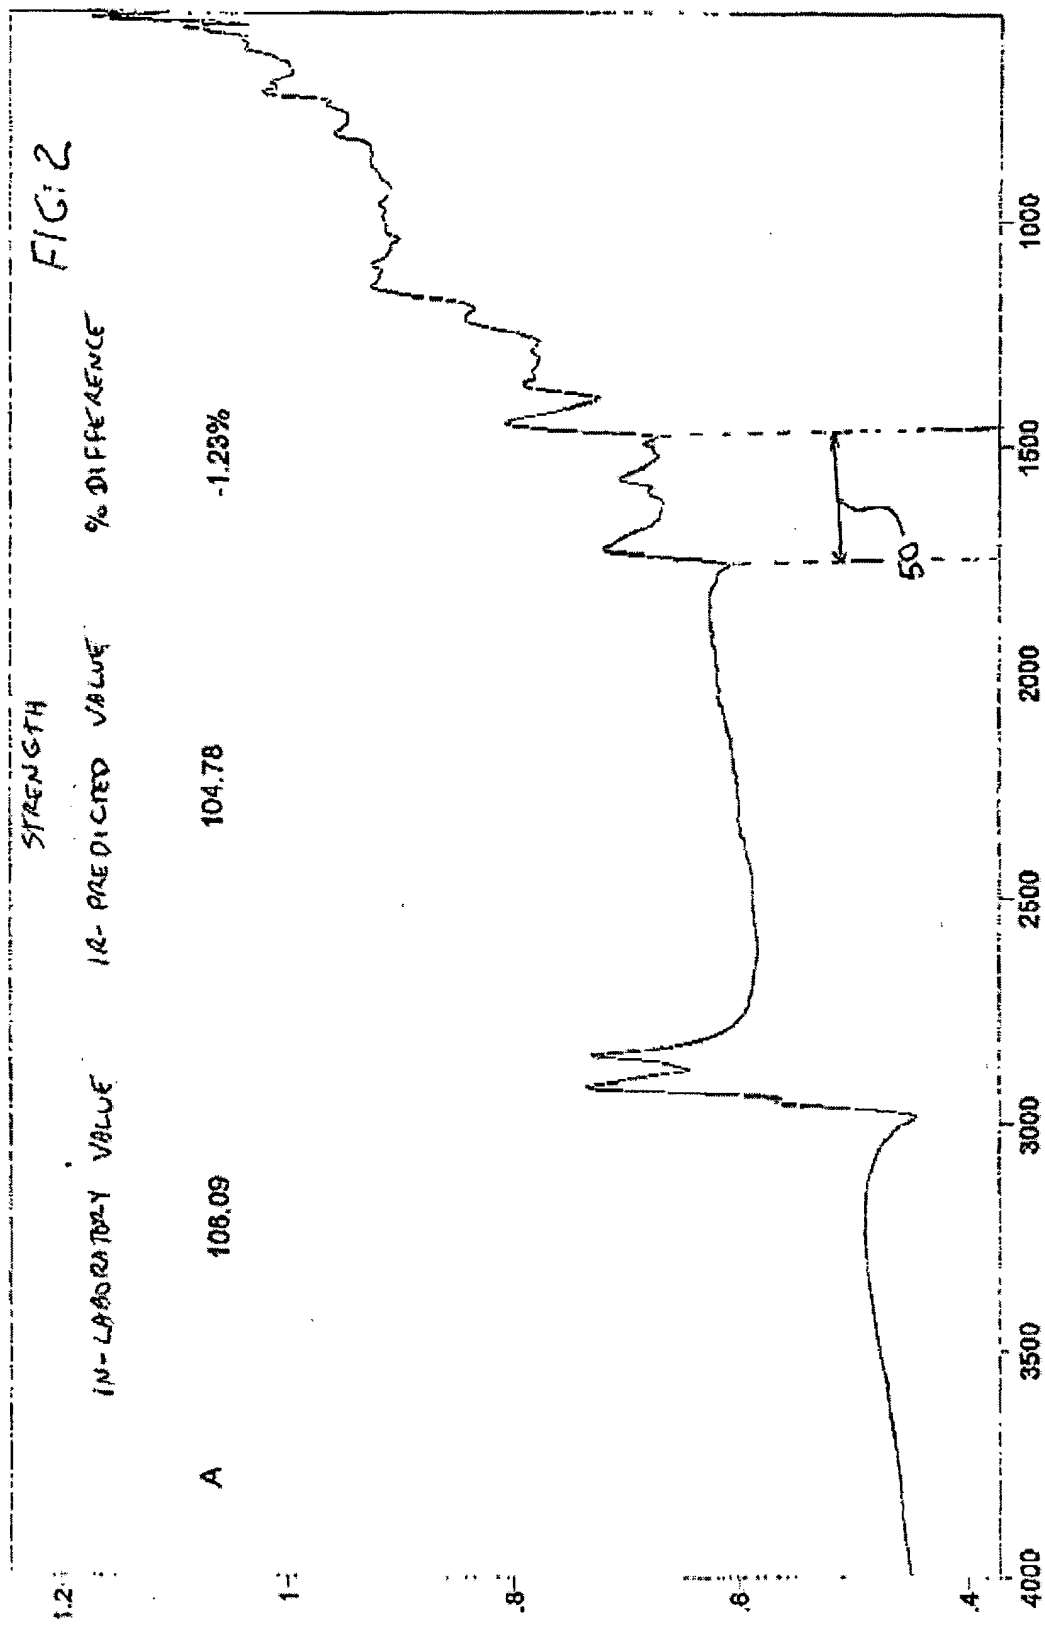

Absorbance / Wavenumber (cm-1)

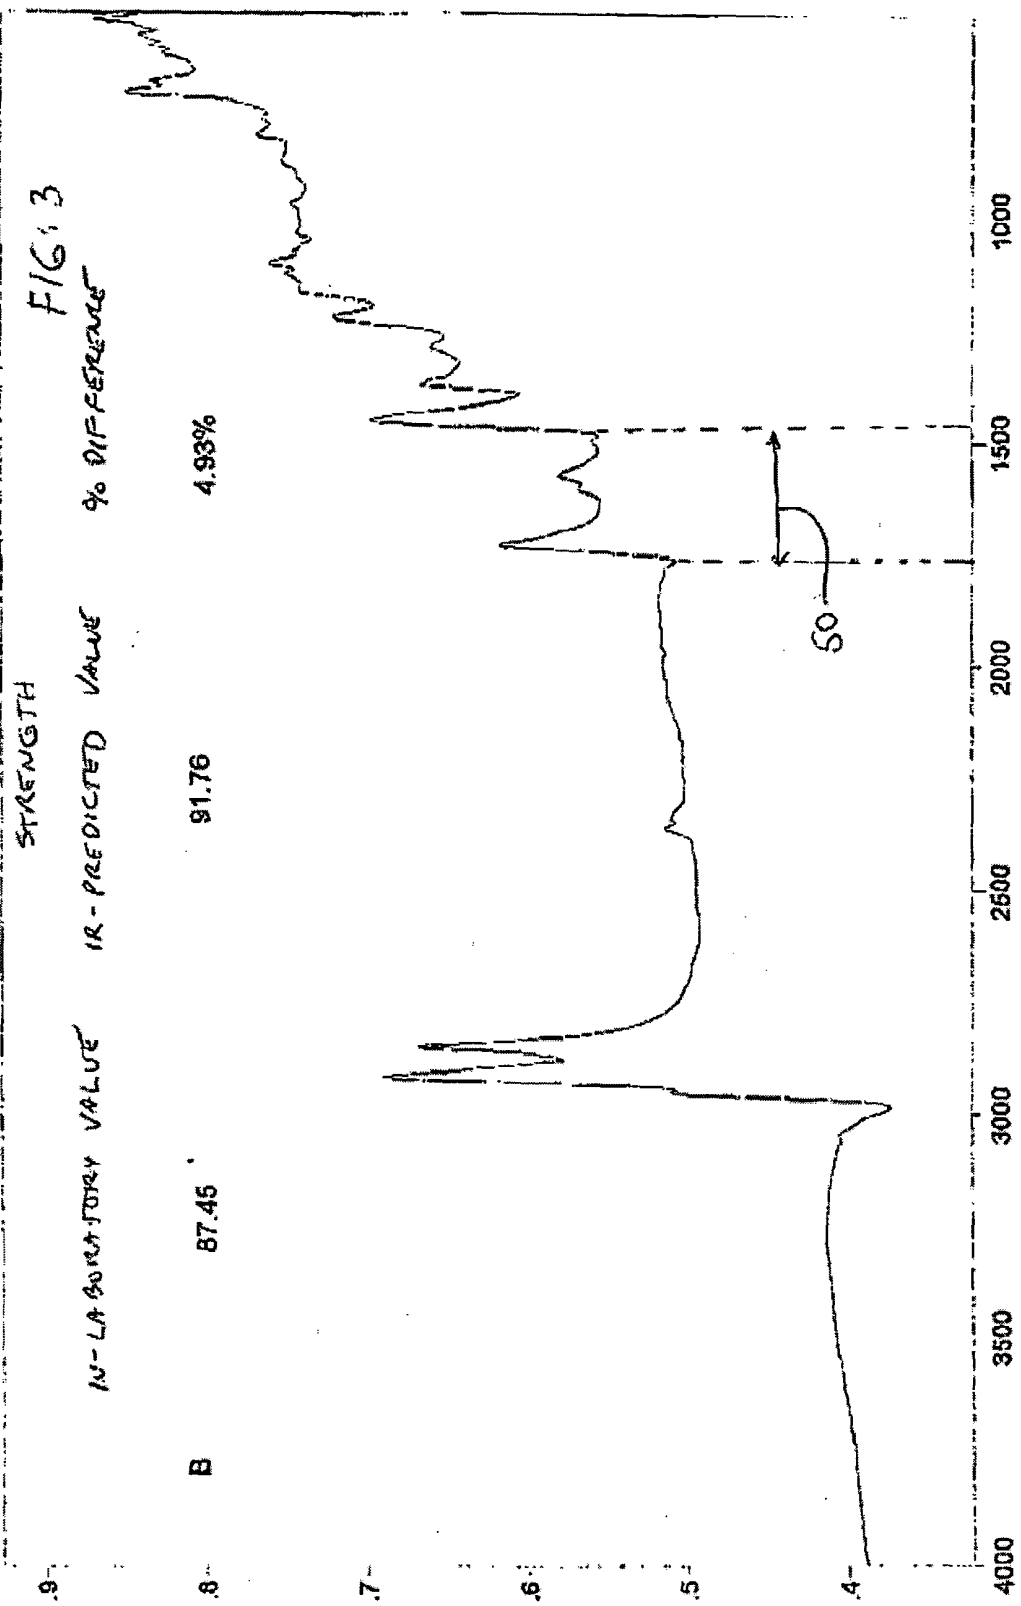

Absorbance / Wavenumber (cm-1)

FIG: 4

STRENGTH

% DIFFERENCE

IR-PREDICTED VALUE

IN-LABORATORY VALUE

1.92%

100.35

98.46

C

1

.9

.8

.7

.6

.5

.4

1000

2000

2500

3000

3500

4000

1782 1485

Absorbance / Wavenumber (cm-1)

50

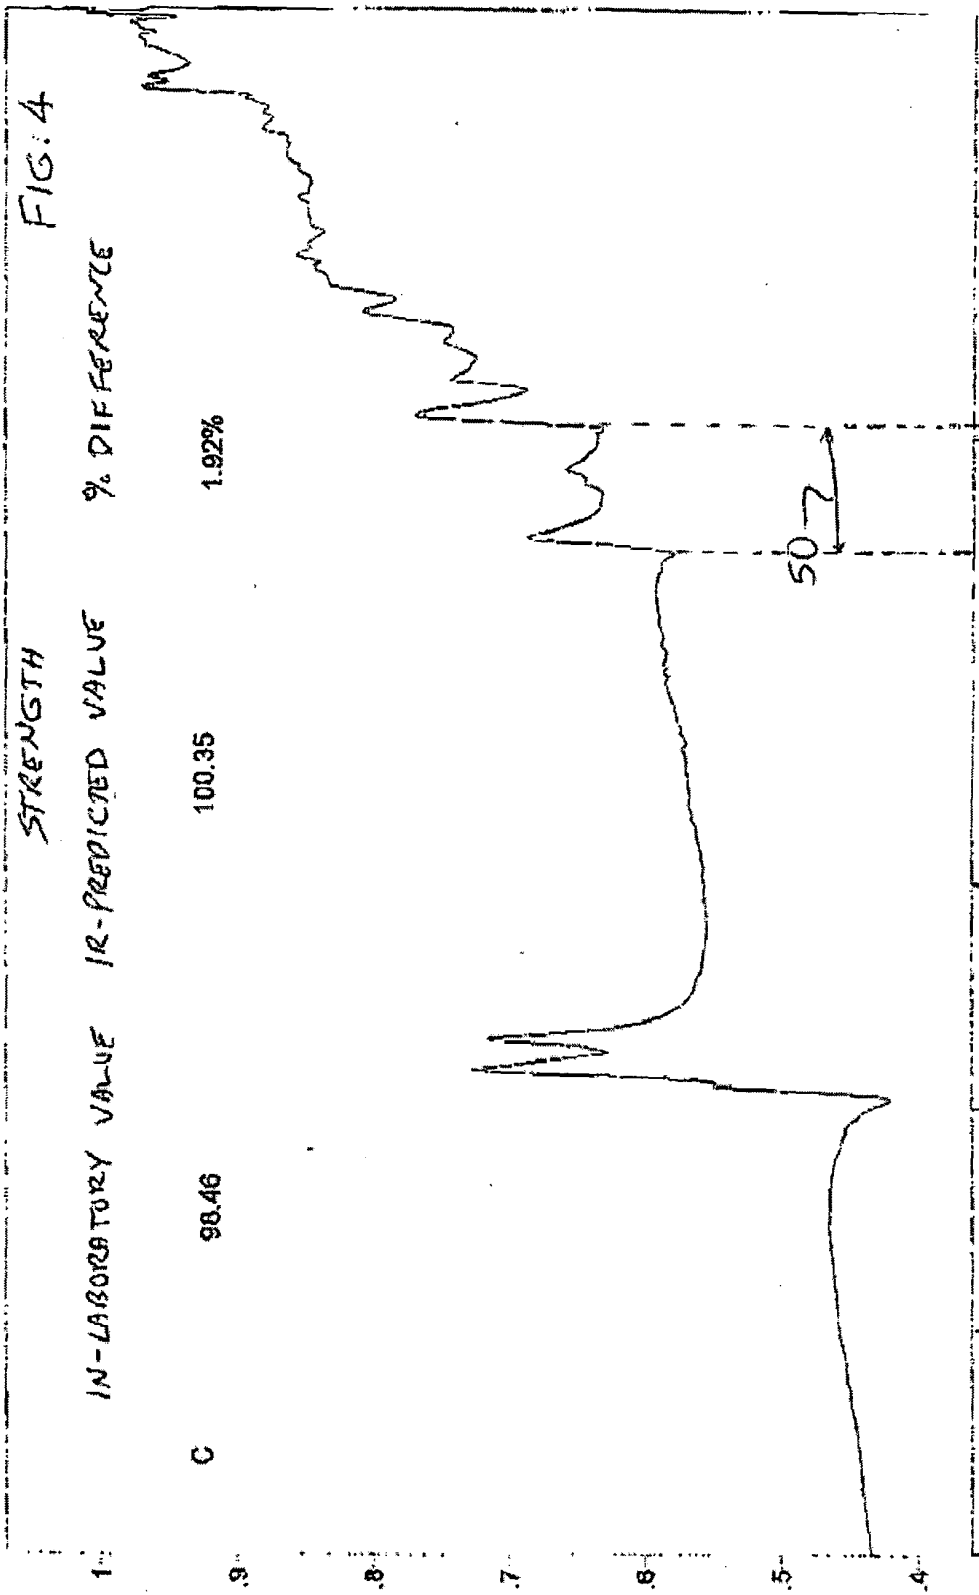


FIG. 5


STRENGTH

IR-LABORATORY VALUES

IR-PREDICTED VALUES

% DIFFERENCE

A	106.09	104.78	-1.23%
B	87.45	91.76	4.93%
C	88.46	100.35	1.92%

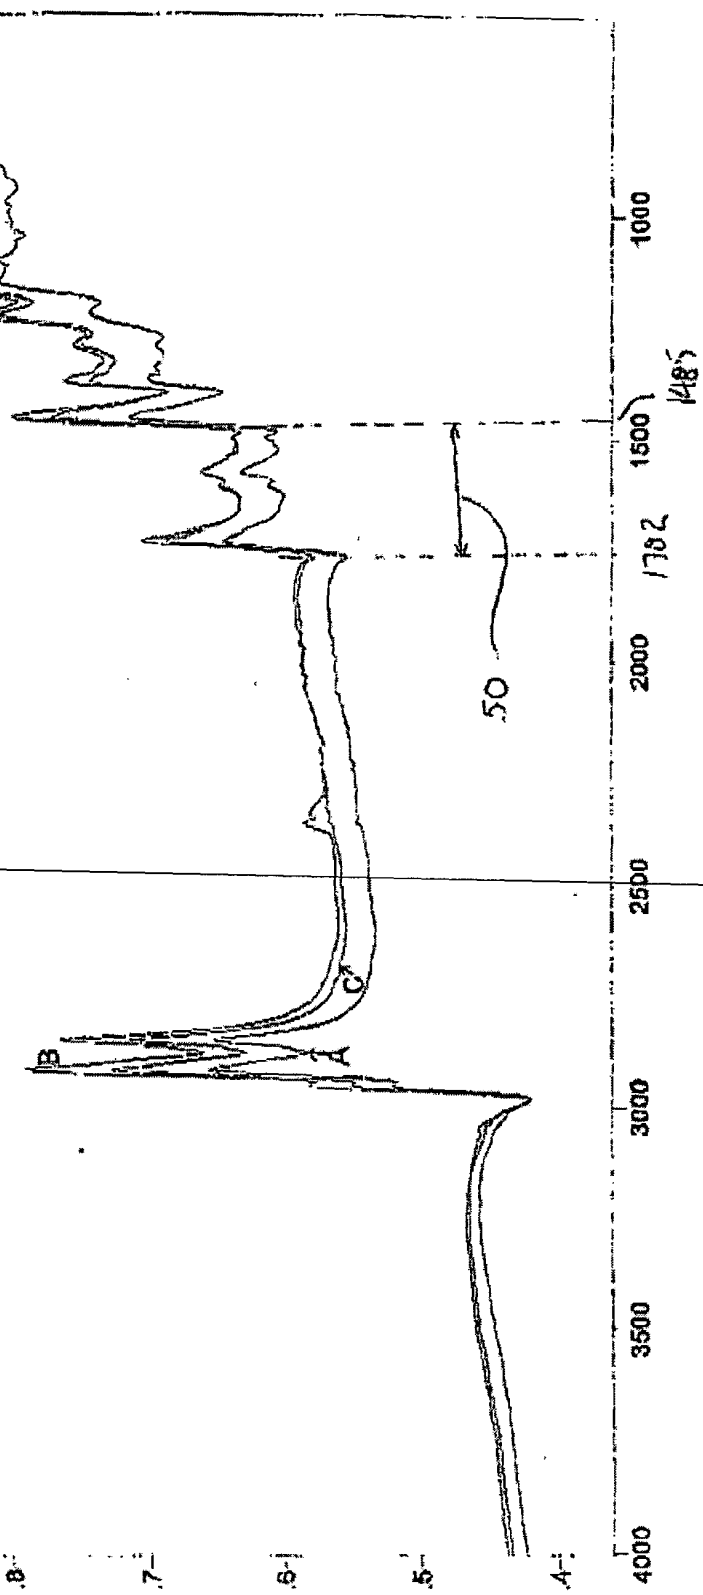

Absorbance / Wavenumber (cm-1)

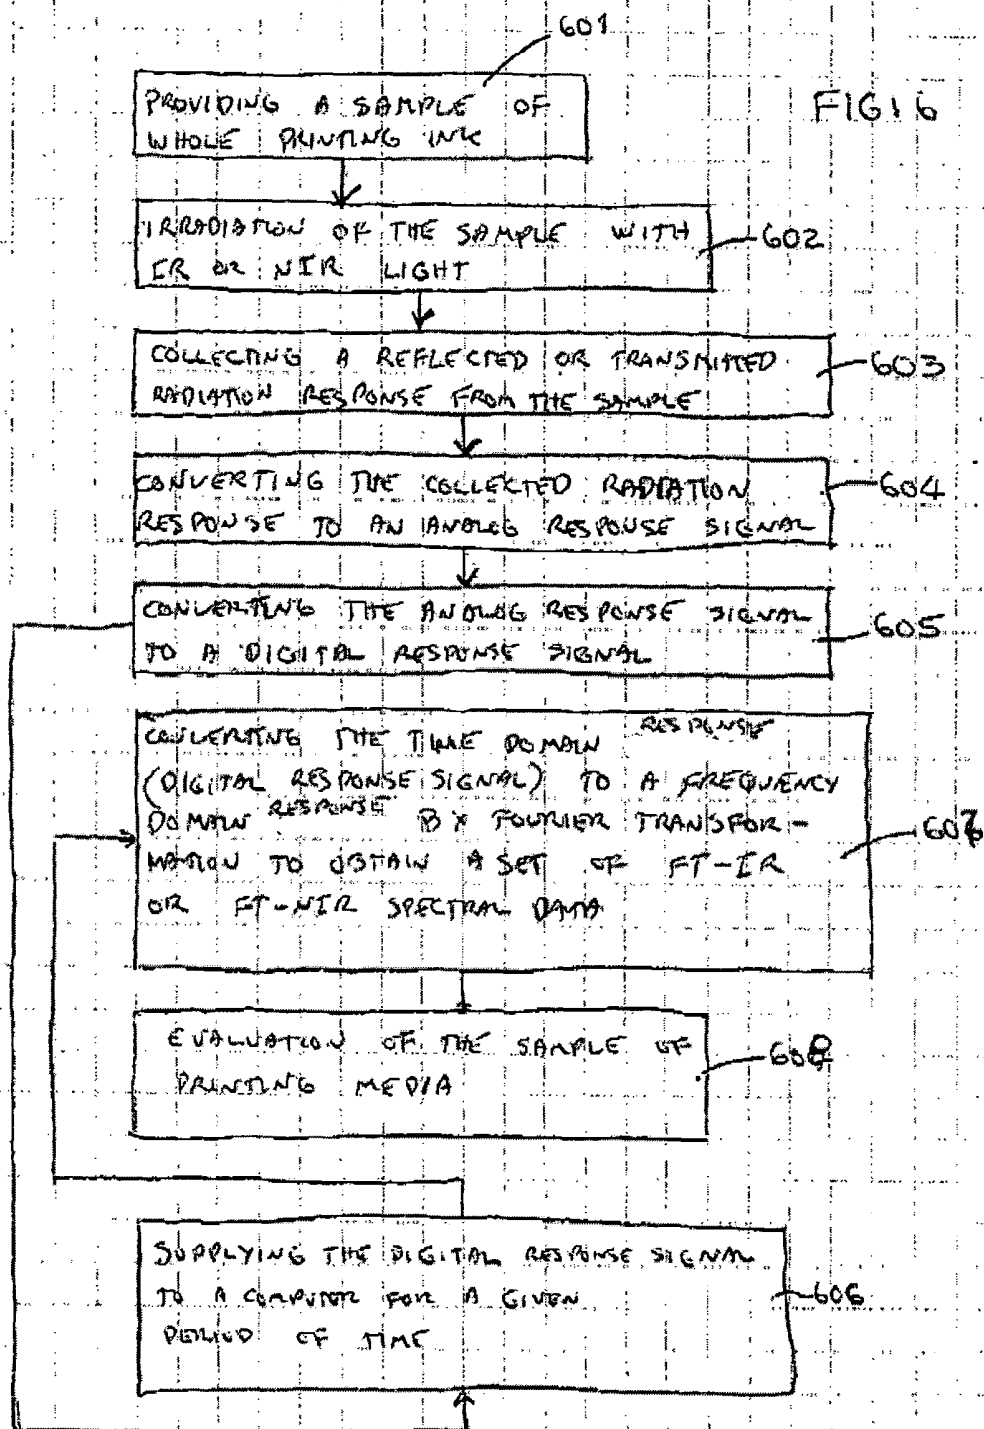


FIG: 7

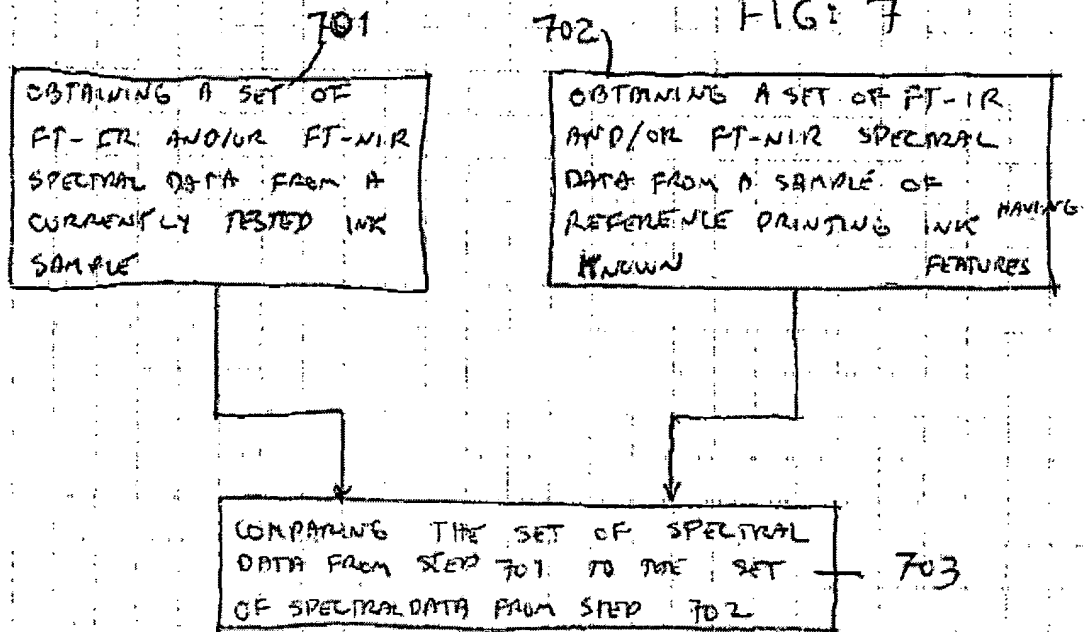


FIG. 8

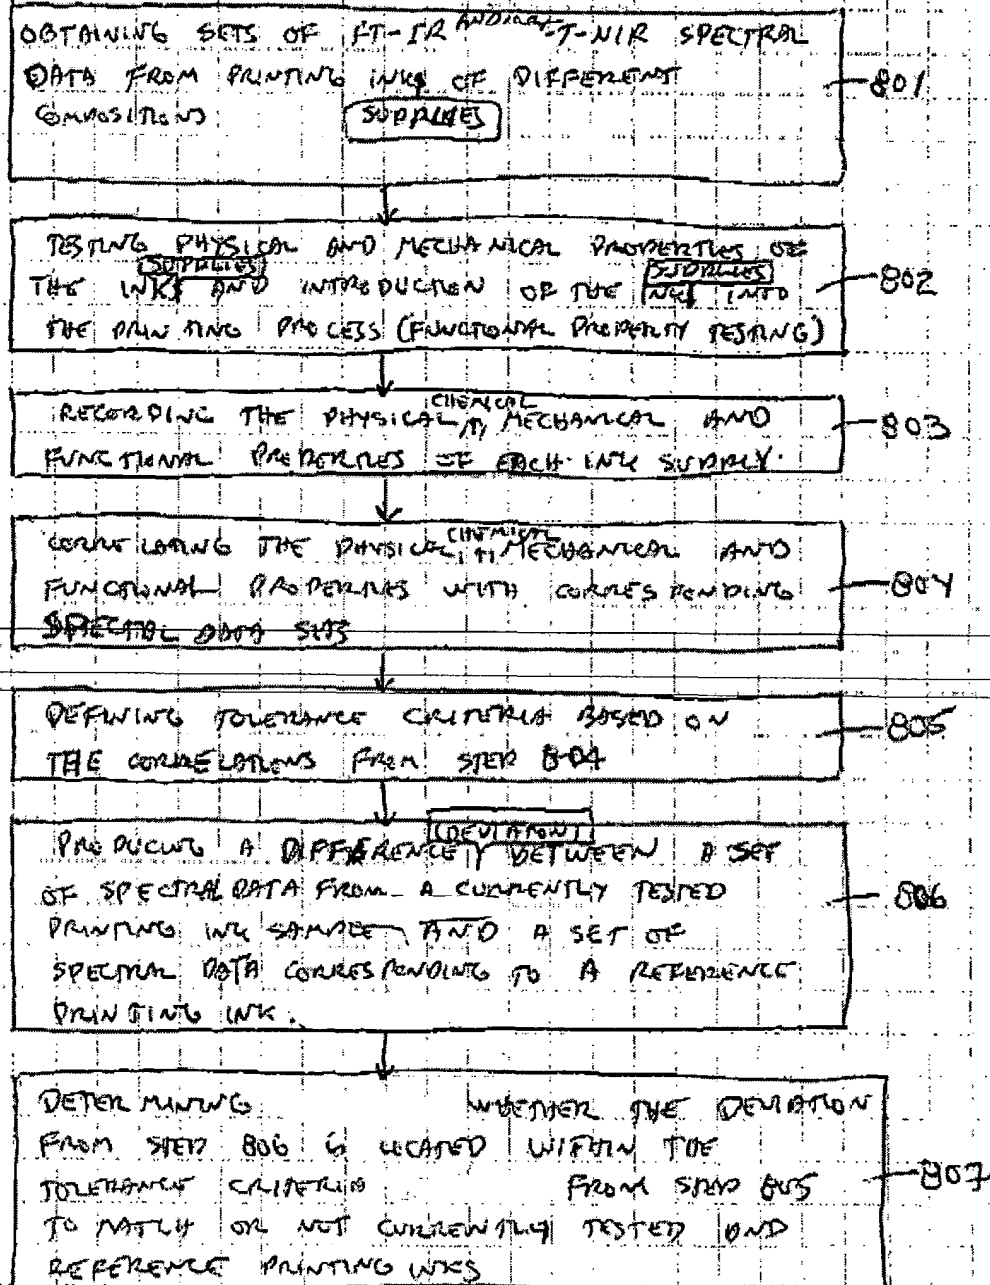


FIG. 9

